

Vetario S30 *Intensive Care Unit*

Operating Manual





Read the instructions before use!



Do not cover!

Danger. Not intended for use with oxygen gas. Use of oxygen creates a fire hazard.

This appliance is only to be used with the mains power supply unit provided with the appliance. Use of another mains power supply unit may cause a hazard. To allow transportation of animals, the appliance may also temporarily be used while attended in a vehicle if connected to a 12 volt accessory socket.

Damaged appliances must not be used.

The appliance, its power supply unit and its supply cord must be placed in an indoor area not subject to splashes of water or wet conditions and protected from or out of reach of animals.

Repairs must be carried out only by a suitably qualified person.

This appliance must not be used, cleaned or maintained by children or persons with reduced physical, sensory or mental capabilities or lack of experience and knowledge without supervision. Children must not play with the appliance.

Disconnect the appliance from the mains power supply during cleaning. Ensure that all electrical parts are kept dry. Avoid alcohol based solutions and make sure that all disinfectant is thoroughly rinsed off plastic parts with clean water. Disinfectant solutions may cause severe cracking of plastic if not correctly rinsed off.

Brinsea Products Inc and its agents or distributors will not be responsible for loss of animals in the event of failure however caused and the user is advised to arrange his own insurance cover where loss of power or mechanical or electrical failure might result in unacceptable losses.


Please read these instructions carefully before setting up your Vetario S30 Intensive Care Unit to achieve best results and keep these instructions safe for future reference.

Your Vetario S30 is designed to allow the user to vary the incubation conditions to suit a wide range of species in different ambient conditions and the specific set-up for every species is beyond the scope of these instructions. There are a range of books and veterinarian texts available covering animal and avian hand rearing and recovery techniques.

To register your new Brinsea product please visit www.brinsea.com within 30 days of purchase and follow the link on the home page to qualify for your free, extended 3-year warranty.

Record your appliance serial number here _____

(see label on carton and chassis)

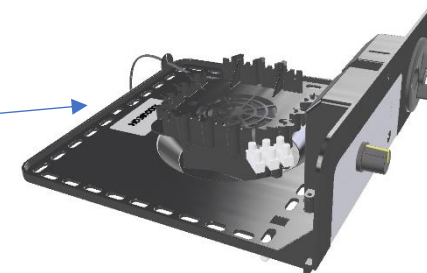

Vetario S30

CONTENTS

1	Unpacking	4
2	Location and Installation	5
3	Functional Features	6
4	Temperature Control	7
5	Small Animal Care	8
6	Cleaning	9
7	Specification	10
	Declaration of Conformity	11

Vetario S30

1 UNPACKING

Your Vetario S30 Intensive Care Unit has been supplied in protective packaging. Please remove all tape, strapping and packing from the incubator and parts. Retain the carton and packing materials to enable the unit to be repacked.

Check that your electrical supply matches that marked on the Power Supply Unit.

The diagram shows all the parts that have been supplied to you. If there are any parts damaged or missing please contact your retailer or Brinsea Products (at the address at the end of the document). **Damaged appliances must not be used.**

1: S30 Intensive Care Unit

2: Power Supply Unit (PSU)

3: Mains power cable

1.



2.



3.



Vetario S30

2 LOCATION AND INSTALLATION

Only use the mains Power Supply Unit supplied with the product. Use of a different mains power supply may cause a safety hazard and will invalidate any guarantee.

Plug the S30 power cable connector into the PSU cable connector.

Plug the mains power cable into the socket on the PSU. Ensure it is pushed fully home in its socket.


Place the PSU and mains cable in a convenient, dry location off the floor and away from animals.

Your S30 will give best results in a heated room free from wide temperature variations and with generous ventilation particularly if several incubators are running at the same time. Ideally thermostatically control the room at between 68 and 77°F (20-25°C). For best results don't allow the room temperature to drop below 59°F (15°C).

S30 Intensive Care Units may be stacked (maximum 2 units high). Ensure the feet of the top unit lock over the 'stacking posts' on the top of the other unit.

TRANSPORT OF ANIMALS

The Vetario S30 may also be used while attended to allow transport of animals in a vehicle. Connect to a 12 volt accessory socket (or cigarette lighter) using adaptor lead part number 15.45 available from Brinsea Products. **It is safest to transport the unit firmly secured in the luggage compartment or firmly secured on the vehicle floor ensuring it cannot interfere with the operation of any vehicle controls. The driver must not be distracted by the animals or S30.**

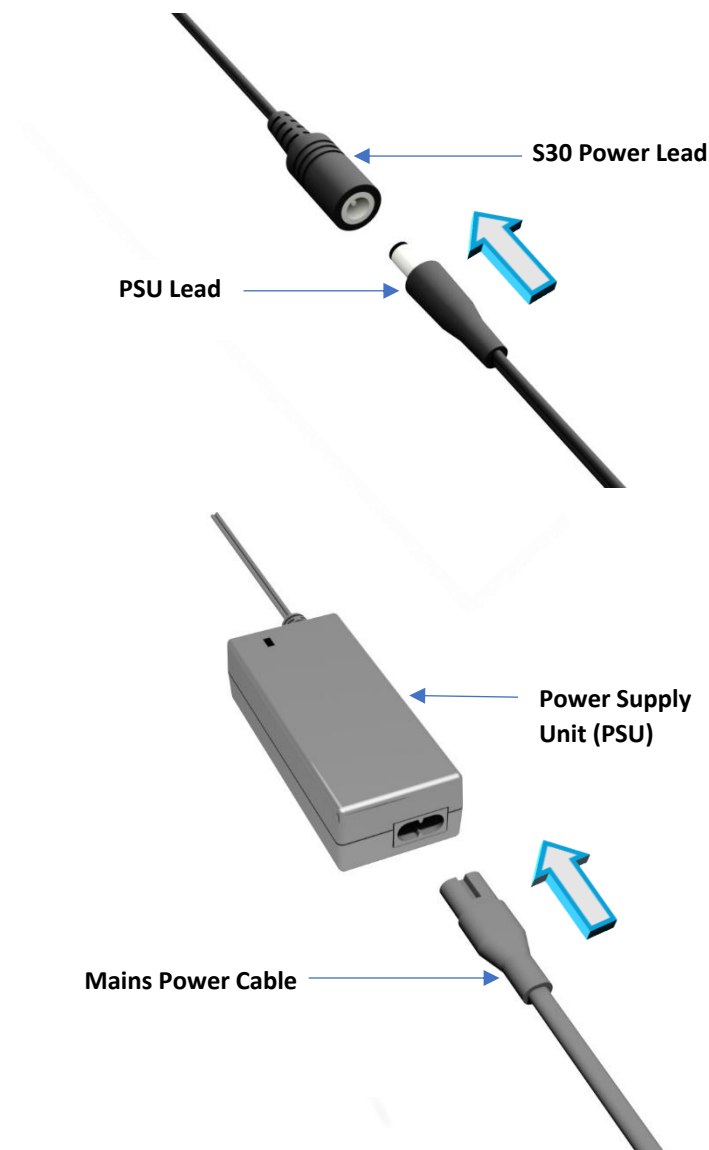

Vetario S30

3 FUNCTIONAL FEATURES

1: Removable Chassis

2: Temperature Control Adjuster

3: Adjustable Air Vent

4: Heating Indicator LED

5: Thermometer


6: Double-walled Cabinet

7: Door

8: Door Latch

9: Integral Carrying Handle

10: Stacking Posts

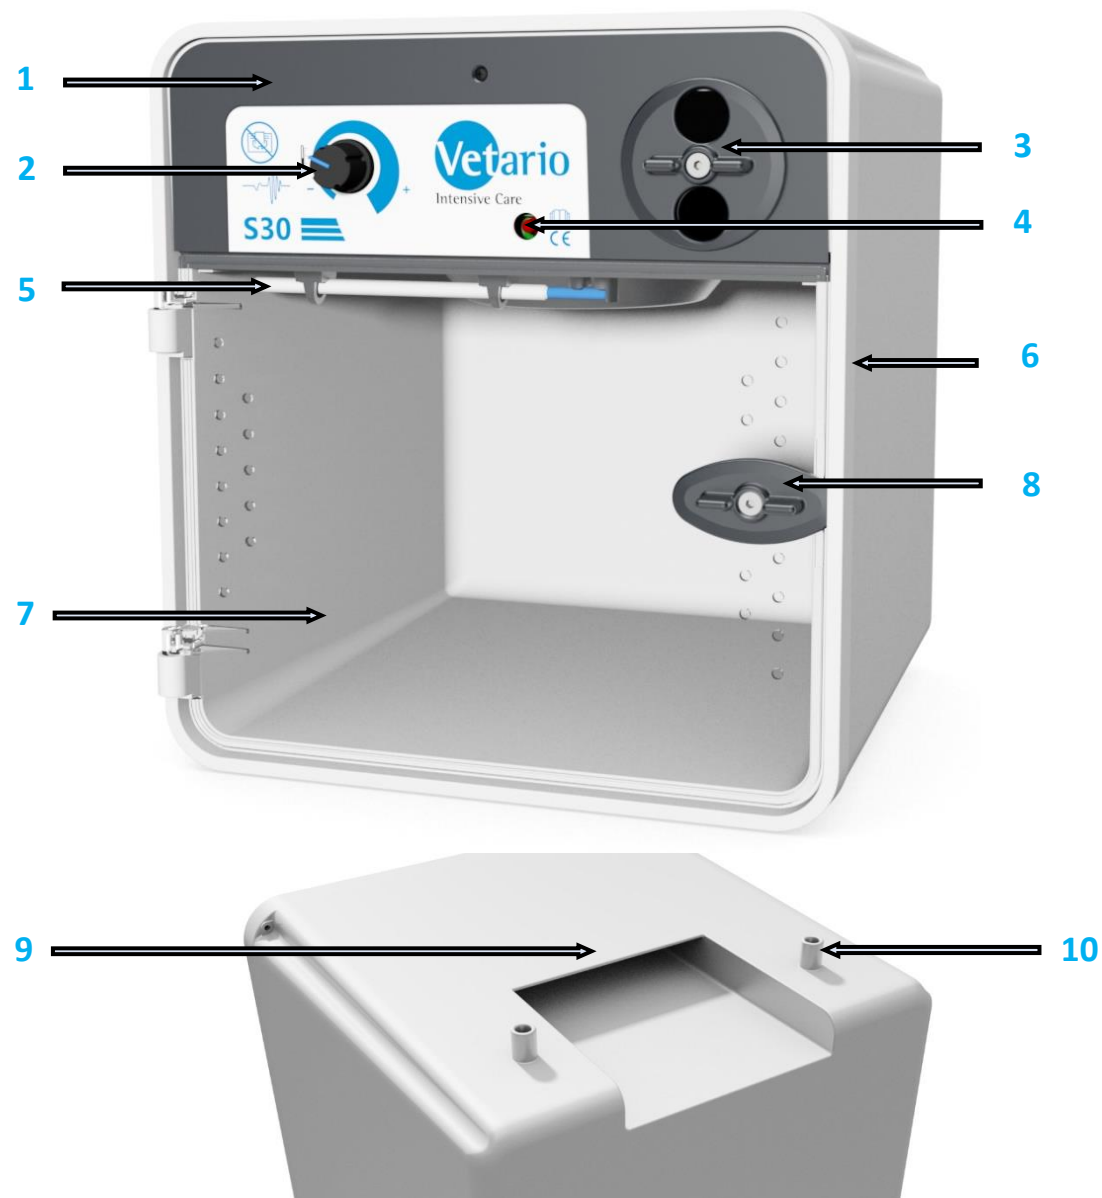

Vetario S30

4 TEMPERATURE

1: The Vetario S30 provides thermostatic control of temperature. To increase the temperature turn the Temperature Control Adjuster clockwise. To decrease the temperature, turn the Temperature Control Adjuster anti-clockwise. See opposite for approximate settings.


2: Check the glass thermometer (located under the Chassis) and adjust the Temperature Control Adjuster to achieve the required temperature. As the S30 warms up and approaches its control setting the LED will change from continuously on, to flashing. If the LED is off, the S30 is cooling. Make small adjustments and check after a few minutes.

3: The S30 will achieve the ideal temperature faster if the Adjustable Air Vent is turned to its closed position (pictured). Afterwards, the vent can be turned to the required setting to give increased ventilation. This may be necessary to maintain low temperature settings in warm environments or if a larger animal is being cared for.

Note that the S30 can only control temperature down to within approximately 10°F (3°C) of room temperature. It cannot cool the air.

Once the correct temperature has been established and the air vent adjusted, the S30 is ready for use.

1.

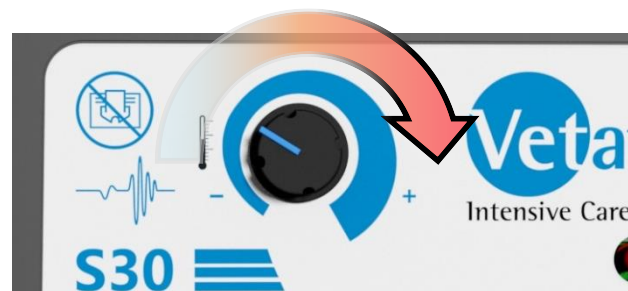

68°F/20°C 82°F/28°C 100°F/38°C
(Approximate settings)

2.



3.



Vetario S30

5 SMALL ANIMAL CARE

Your Vetario S30 has been specifically designed for the care of injured or sick small animals. Animals should always be cared for following the instructions and advice given by your veterinary surgeon.

The first stage of treating a cold animal (hypothermia) is to prevent further heat loss, by wrapping the casualty in insulating materials such as blankets, bubble wrap or silver foil. It is recommended to pre-heat the S30 and allow the temperature to stabilise before adding young birds or small animals. If you are aware of an incoming animal patient, the S30 may be switched on so that it is ready for immediate use when the patient arrives.

Once the S30 is warmed to the correct temperature the animal can be transferred. The amount of bedding should be reduced at this stage to allow warming from the environment in the S30. All animals will benefit from some bedding in the bottom of the cabinet such as an absorbent pad to help reduce soiling. Small animals such as fox or badger cubs can benefit from having a soft toy for company while single ducklings or pheasant chicks can be provided with a safe mirror. Wild animals may become very distressed when handled by humans. Place the S30 where there is minimal disturbance.

All small mammals and birds will benefit from being kept in an environmental temperature within their 'thermoneutral range'. This is the range of temperatures in which an animal expends no energy to maintain its body temperature. The thermoneutral temperatures for typical adult mammals and birds are given in table 1. For birds, the thermoneutral range depends upon size, with smaller birds requiring higher temperatures. Reptiles and amphibians should be kept within an 'activity temperature range' (ATR) in which it can control its body temperature. ATR values for typical reptiles and amphibians are also given in table 1.

Hypothermic adult animals should be warmed in the S30 set to their thermoneutral range. The temperature of both the S30 and the animal should be recorded at regular intervals. Careful monitoring and observation of the animal should be undertaken to ensure that it is not showing signs of distress. i.e. panting or shivering. These animals are also likely to be dehydrated and/or 'shocked' (hypovolaemic) so warming alone will not correct these things and may make them worse. All adult animals must therefore be provided with adequate fluid therapy at the same time as warming and veterinary care (in person, over the telephone or in written Standard

Operating Procedures). Injured animals also require pain relief (analgesia) which can be prescribed by a veterinary surgeon.

If the animal will drink, then an oral rehydration fluid can be provided in a shallow bowl. If the animal will not, or cannot drink, then fluid must be given in other ways. In birds, rehydration fluids can most easily be provided by crop tubing, provided the bird can lift its head and swallow. In mammals, intravenous or intraosseous fluids are usually required to rehydrate patients. These must only be administered by a veterinary surgeon or veterinary nurse.

Only feed a poorly animal once it is warm and always start with liquids only. Do not place moist, solid food in the intensive care unit as it will rapidly go bad due to the warm environment.

Dependent animals (those that would naturally be in a nest) should be kept in the S30 set at 82-90°F (28-32°C) until they are of an age where they can maintain their own body temperature when the heat can be reduced to the thermoneutral range for that species. Carefully observe their behaviour for signs of panting or shivering to help determine the best temperature for them at that stage. Very small baby animals may require an artificial fabric 'nest' to be created in the S30, lined with paper towel.

Like adult animals, baby animals are frequently dehydrated upon arrival and should be fed with an oral electrolyte solution. They also frequently have a low blood glucose level (hypoglycaemia) and should be fed appropriately soon after the initial electrolyte feed. If the animal is unable to lift its head, and/or swallow, then it will need to be given fluids and glucose by injection – this should be under veterinary direction.

Table 1. Typical thermoneutral and active temperature ranges (ATR)

Species:	Temperature range:
Mammals	59 – 68°F (15 – 20°C)
Medium and Large Birds	59 – 77°F (15 – 25°C)
Small Birds	68 – 86°F (20 – 30°C)
Very Small Birds	77 – 95°F (25 – 35°C)
Reptiles	68 – 86°F (20 – 30°C)
Amphibians	59 – 86°F (15 – 30°C)

Vetario S30

6 CLEANING

Disconnect the Power Supply Unit from the mains supply.

Do not immerse the cabinet. It may be cleaned further by separating the inner and outer parts. Do not over-tighten the fixing screws.

Never wash the cabinet parts in liquids over 50°C (120°F). Do not use a dishwasher to clean any parts.

Always rinse thoroughly as cleaning agents / disinfectant may damage plastic after prolonged contact. Avoid solutions containing alcohol.

Following each use of your S30 remove all debris from the floor. Wipe all internal surfaces clean with a damp cloth soaked in a water-based disinfectant solution (diluted according to the manufacturer's recommendations). Rinse surfaces thoroughly with a cloth made damp with clean water.

The exterior of the S30 may also be cleaned with a damp cloth with disinfectant solution and then rinsed off thoroughly.

To disassemble:


1: Open the door to at least 90 degrees. Lift the door up (as pictured) to remove it from the cabinet hinge loops.

2: Remove the chassis by pressing at the location shown in an upwards direction whilst sliding the tray out towards you. The power lead can be pulled through the cable hole.



3: To re-assemble; fit the S30 power lead through the hole in the back of cabinet and gently pull through.

4: Slide the chassis back into position and 'click' back into place. **Ensure that the power lead is taut while sliding the chassis into place to prevent the lead being damaged / trapped.**

5: Re-fit the door by sliding the doors hinges down into the cabinet's hinge loops.

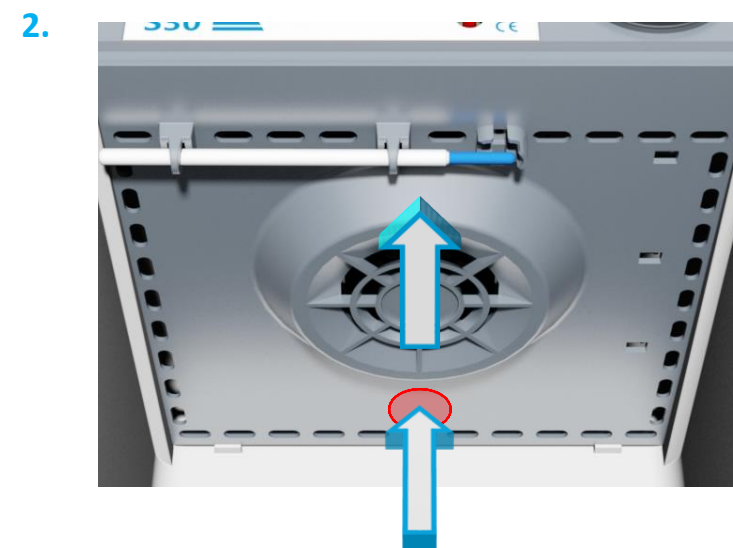

PRESS HERE AND SLIDE FORWARD

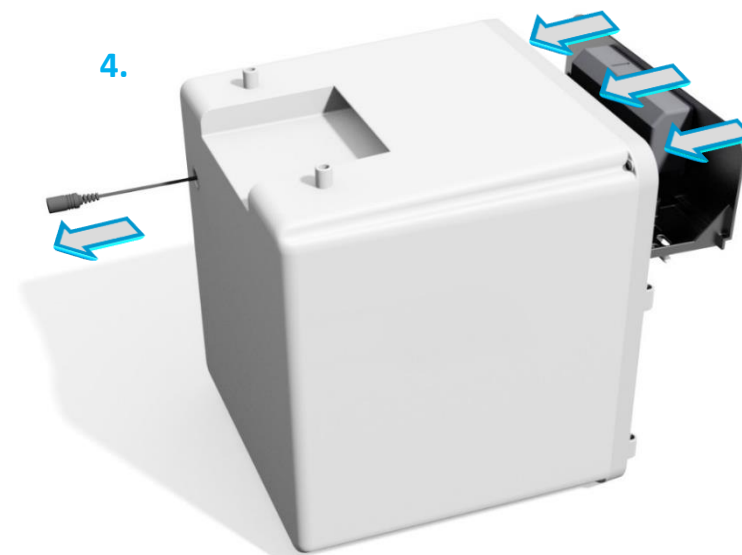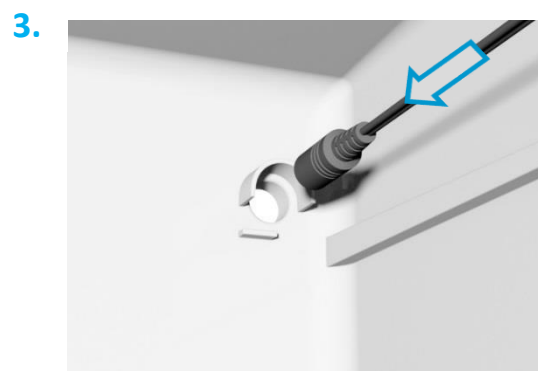

Vetario S30

7 SPECIFICATION

Overall Height:	11 ¾ inches (297mm)
Overall Width:	10 ½ inches (270mm)
Overall Depth:	10 ¾ inches (275mm)
Floor Area:	9 ⅓ x 9 ⅓ inches (240mm x 240mm)
Effective volume:	2.5 gallons (9.5 litres)
Weight:	4.6lbs (2.1 Kg)
Power Consumption:	
Maximum	36 Watts
Typical average	18 Watts
Electrical Supply:	115V, 50/60Hz.

Brinsea Products Inc.
704 N Dixie Ave., Titusville, FL 32796-2017 USA
Phone. (321) 267-7009 Toll Free 1-888-667-7009
e-mail: support@vetario.com, website: www.vetario.com